

11/1/6

2 → Variable orifice valve arrangement.
 6. Constant respiratory pressure transducer

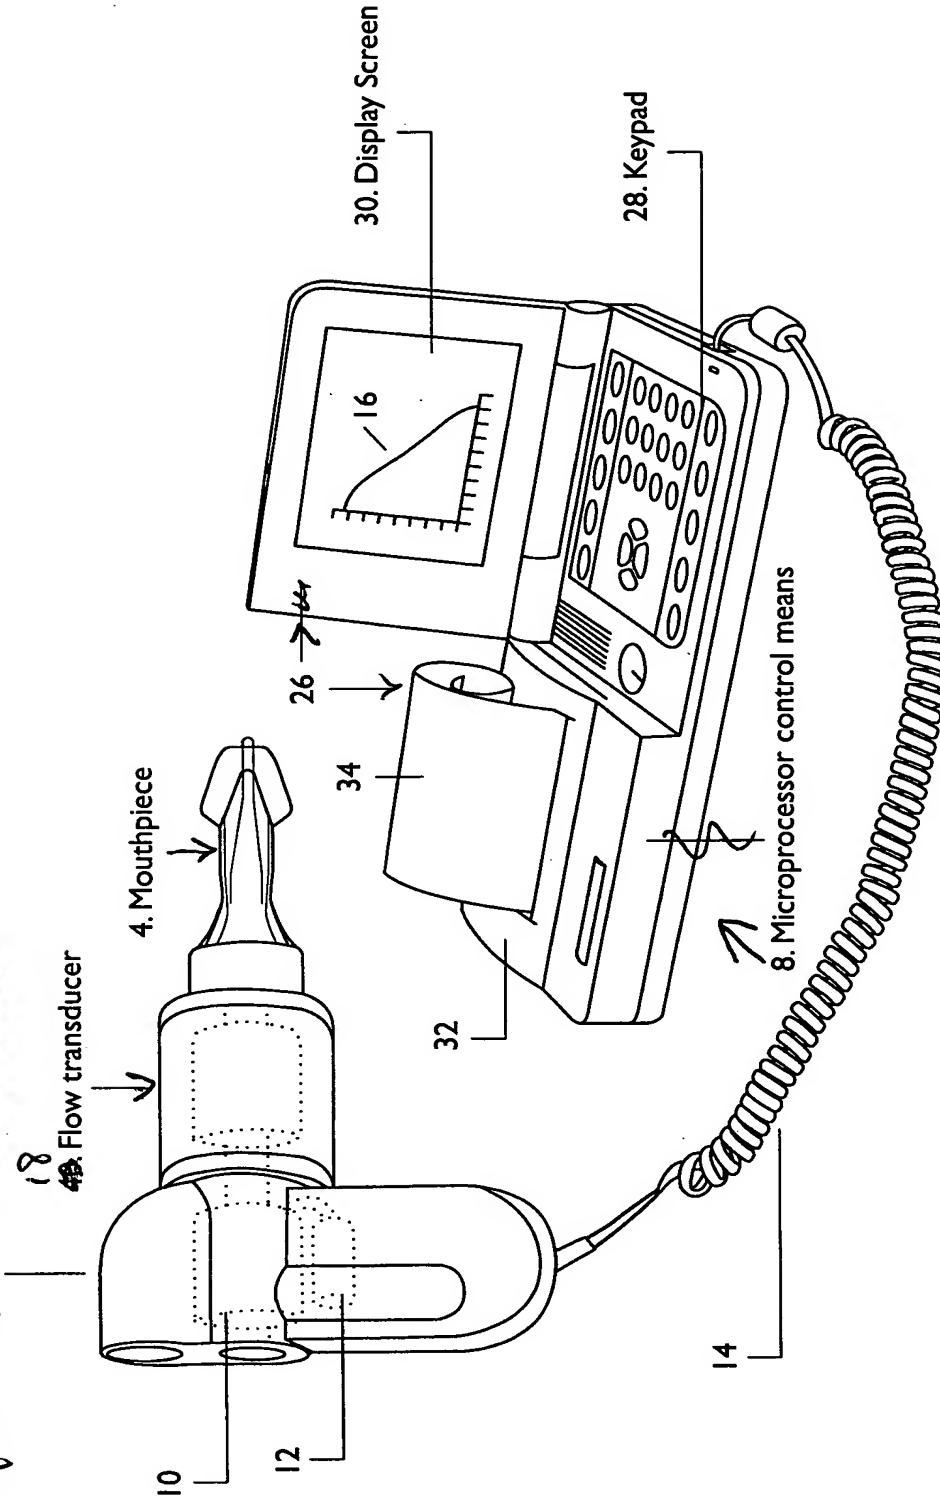


FIG 1

2/4 2/6

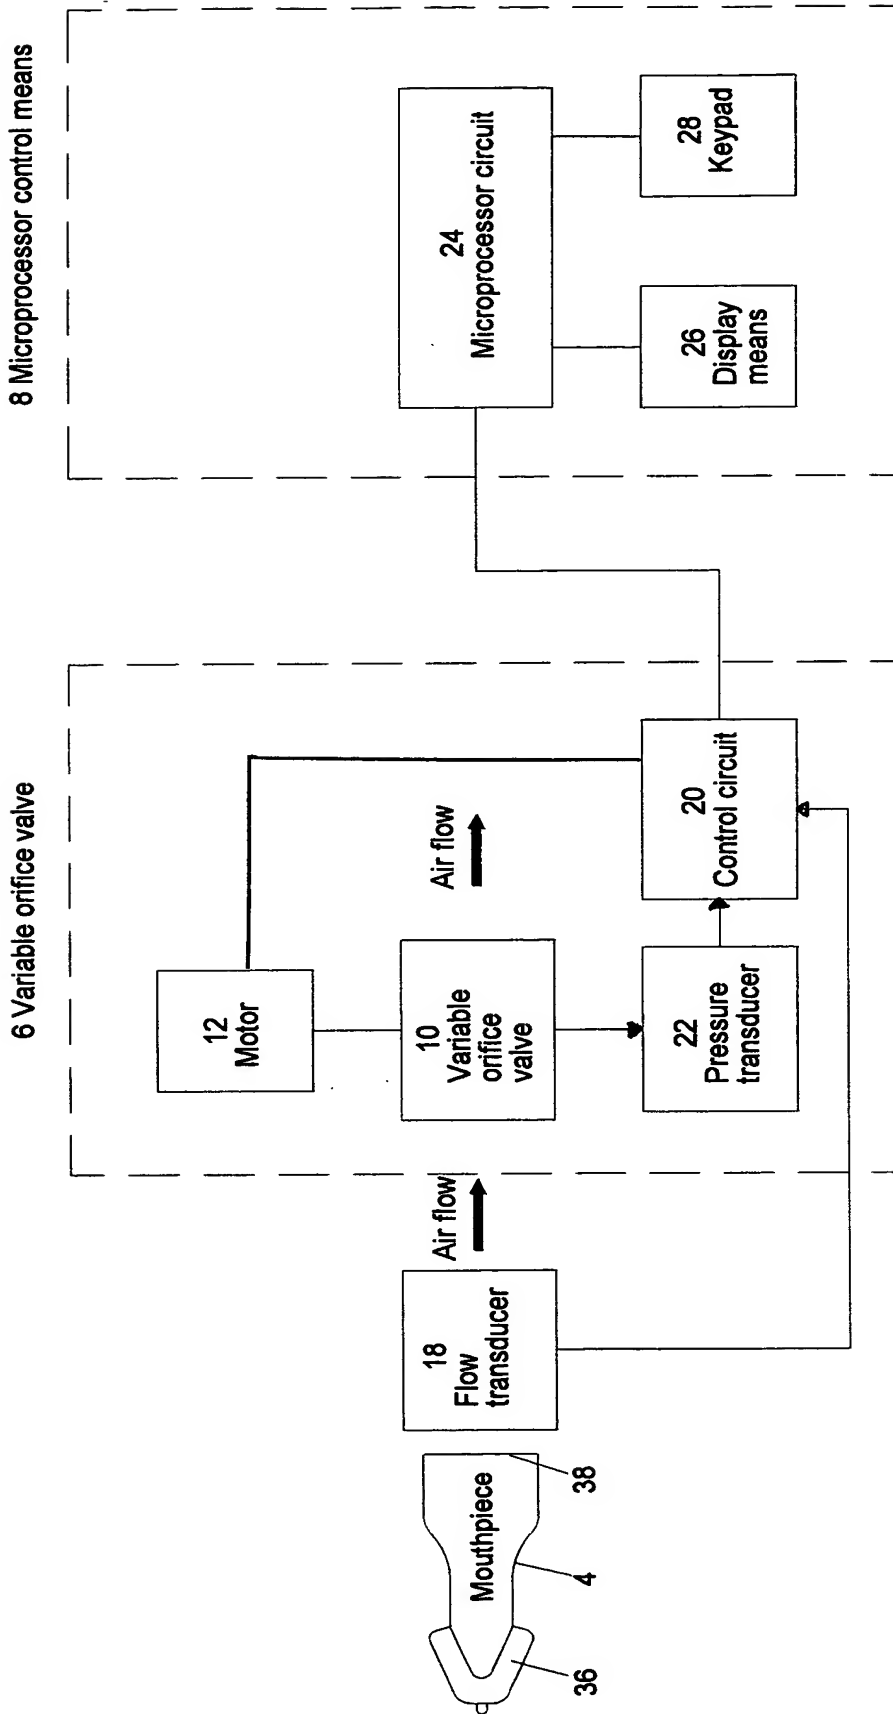


FIG 2

2/1 3/6

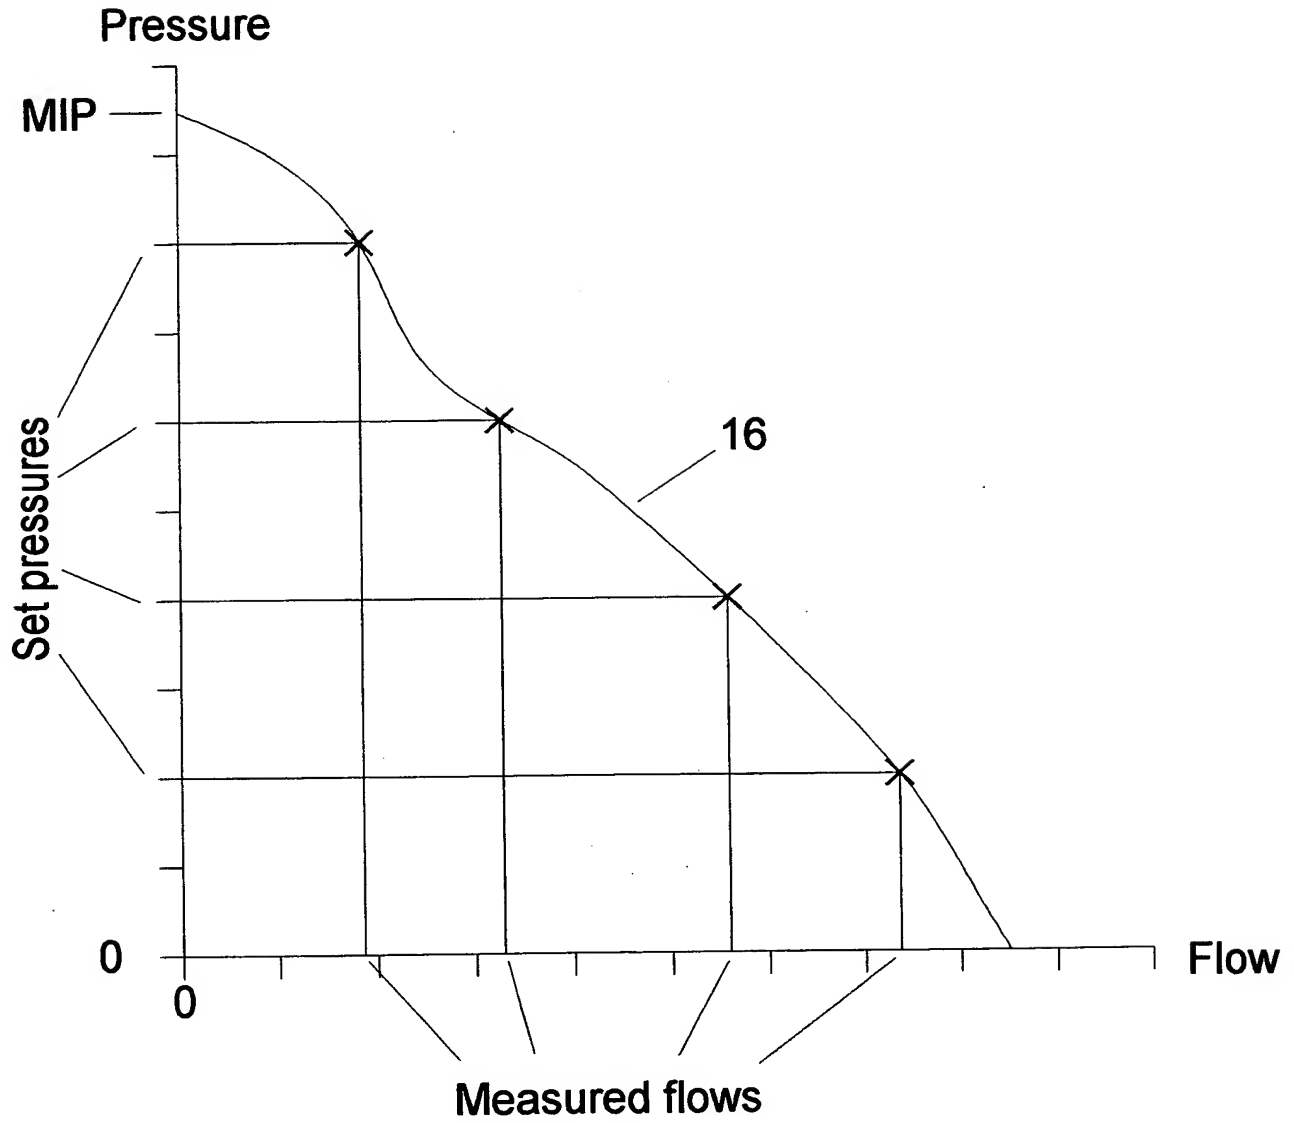


FIG 3

~~4/4~~ 4/6

Rotary variable orifice valve


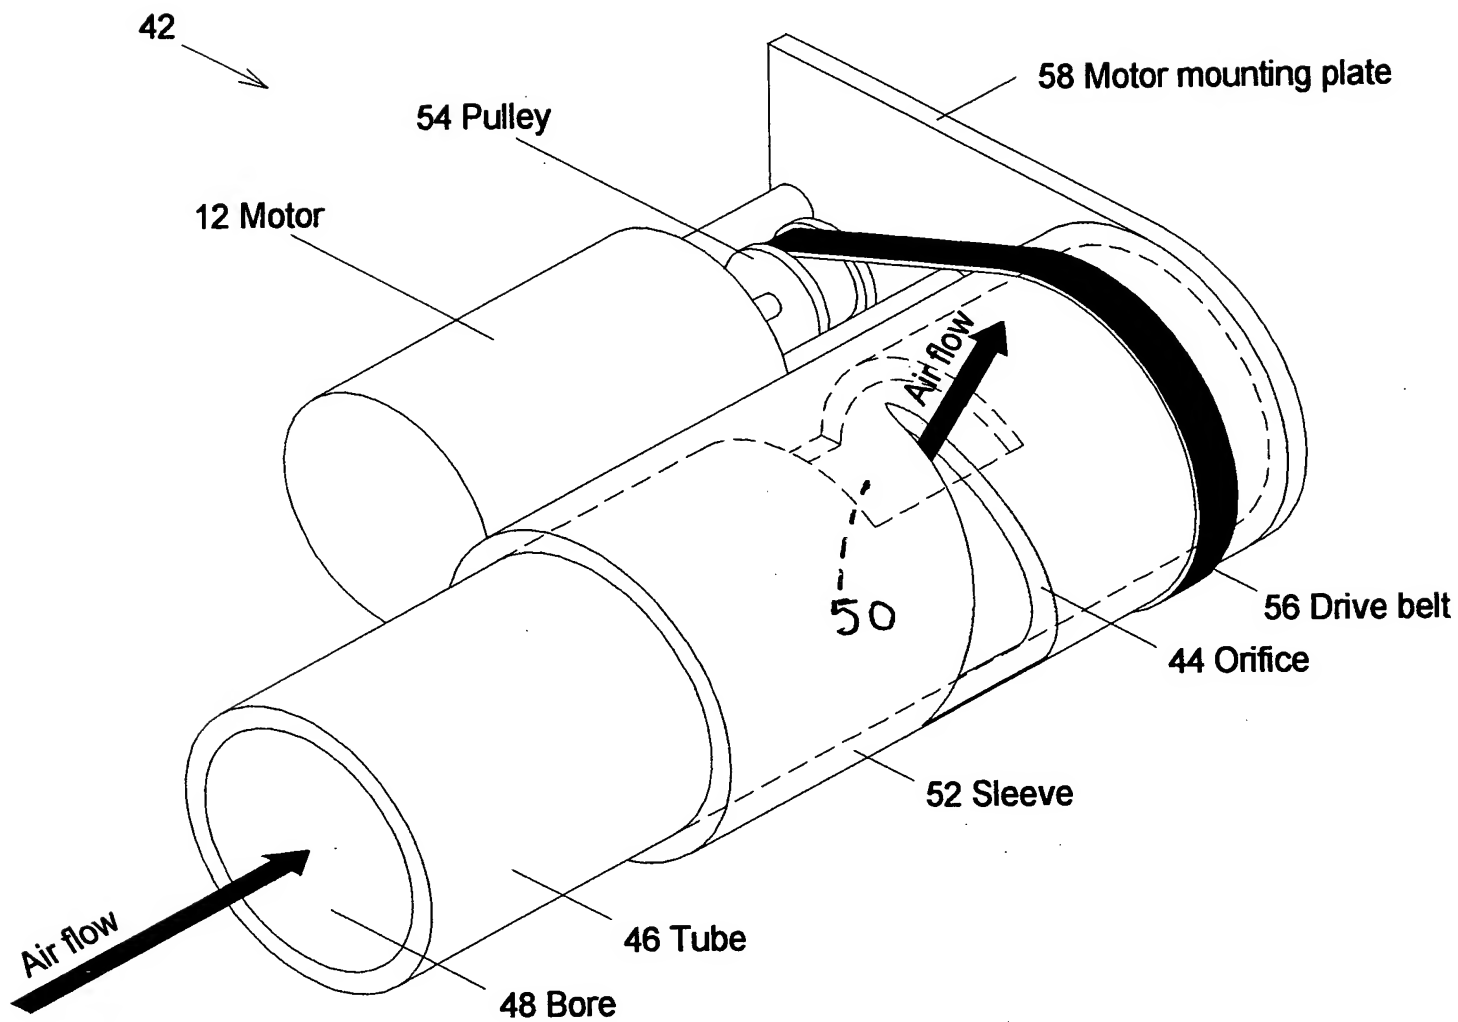


FIG 4

5/6



6/6

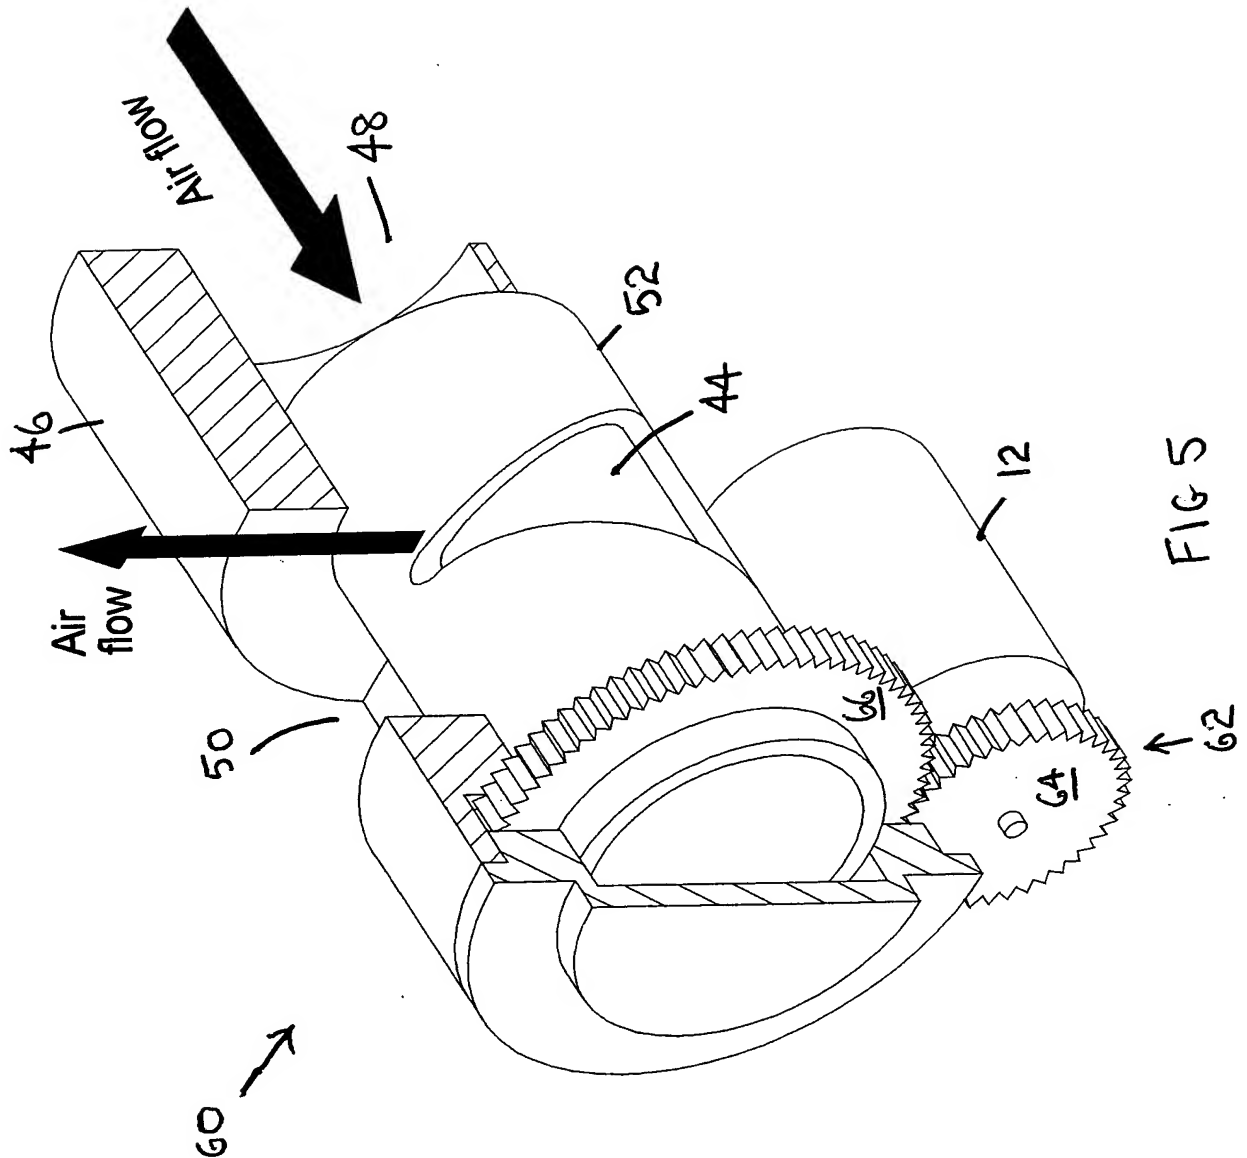